

### TV2500

ASTM D445 - ASTM D446 - IP 71 - ISO/EN 3104 - ASTM D1298



- ⊕ **Stainless steel**
- ⊕ **Compact, small foot print**
- ⊕ **Levelling feet for spirit level**
- ⊕ **RS232 communication**
- ⊕ **Two decimals readout (0.01°C)**
- ⊕ **Cooling coil**
- ⊕ **Fluid level detection (float)**

#### General

The TV2500 is specially designed for tests that require precise temperature control like the determination of kinematic viscosity and sensor or thermometer calibration. The visibility through the bath is excellent.

The stainless steel construction ensures stable temperature control, which is further improved by a special stirring mechanism. The bath is fitted with adjustable feet for leveling. The cover of the bath has four round ø51 mm openings with lids, for suspending glass capillary viscometers in holders.

#### Span

The TV2500 operates from ambient .. +120°C (242°F). Sub-ambient temperatures can be achieved when using the built-in cooling coil in combination with tap water or a Tamson TLC10-3 cooling circulator. Built up of condensate may limit the practical use to about +5°C.

Item	Unit	TV2500	
P/N		19T1003	
230V/50~60Hz			
P/N		19T1004	
115V/60Hz			
Power	[kW]	1.5	1.5
Heat rate water	[°C/min]	0.8	
Heat rate oil	[°C/min]	1.9	
Heating	[kW]	1.4	1.4
Used materials inside bath		Stainless steel, brass bearings	
Range		Ambient..120°C Ambient..248°F	
Reading	[°C/°F]	Menu selectable	
Setting ±	[°C/°F]	0.01	
Stability ±	@50°C	0.02°C Water	
	@100°C	0.02°C Oil	
Bath volume	[L]	25	
Top lid		Removable with four ø51 mm holes	
Opening bath	[mm]	185*155 (effective use)	
Depth	[mm]	300	
Length	[mm]	370	
Width	[mm]	204	
Height	[mm]	600	
Weight	[kg]	15	
CE		All models conform to CE regulation	

#### Software

Use the standard RS232 interface and free TamCom® software to set parameters, program a temperature curve or log the bath temperature.

#### Accuracy

The set point is adjustable in steps of 0.01°C. The overall system accuracy and homogeneity are better than ± 0.02°C, specified with water or oil during a measuring period of one hour.

#### Temperature readout

Available in °C or °F.

#### European Pharmacopoeia

Using Ubbelohde viscometer tubes, the bath conforms to the "Pharmaceutical 2.2.9, capillary viscometer method".

### TV2500

#### Accessories


#### Safety

The bath conforms to CE regulations. It further is equipped with a mechanical adjustable and automatic over temperature safety thermostat to guarantee safe around the clock operation. When working above 50°C the safety window is advised to be used. The TV2500 is also equipped with a float to warn the user with an acoustic signal when the bath fluid is too low.

#### Safety Window

When using the TV2500 at higher temperatures it is advised to mount a safety window. The safety window protects the user from heat radiating from the inside window.

When using the safety window, the user sitting in front of the window is protected against heat and fluid, in the very rare case the window might break. All our windows are made of very tough hardened glass. Use of a spill tray is also recommended to keep your lab clean. Dripping fluid from glass capillary viscometer or accidental spill during refilling the bath fluid is collected. The tray is provided with a 3/8" BSP inner thread valve.

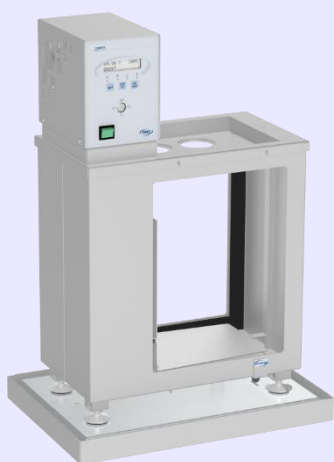
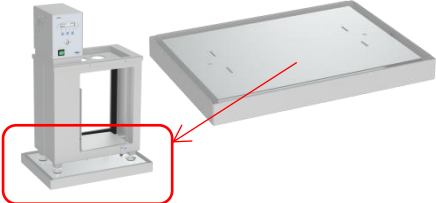







TV2500 is standard included with:		
P/N	Picture	Description
23T2407		Cover with 4 openings: - 4 x ø51 mm opening - 2 x ø12.5mm opening for thermometer
		4 * lid for ø 51 mm opening

Optional cover for TV2500:		
P/N	Picture	Description
23T2408		Cover with 3 openings: - 3 x ø60 mm opening - 2 x ø12.5mm opening for thermometer
		3 * lid for ø60 mm opening






### TV2500

#### Accessories

Accessories		
P/N	Picture	Description
02T0210		Glass safety window with clamps. For use at temperatures above 50°C.
02T0200		Spill tray. Protects your lab against dripping and spilling during operation or when replacing bath fluid. The tray has a drainage with valve and 3/8" BSP connection.
00T0909		Illuminator "Z41" stand alone (85 ~ 230V/50-60Hz)
00T0050		Cooling circulator TLC10-3 - 230V/50Hz
00T0051		Cooling circulator TLC10-3 - 230V/60Hz
00T0052		Cooling circulator TLC10-3 - 115V/60Hz
00T0565		Cooling circulator TLC15-5 - 230V/50Hz
00T0567		Cooling circulator TLC15-5 - 230V/60Hz
00T0570		Cooling circulator TLC15-5 - 115V/60Hz
12T1075		Tubing with connectors and clamps to be used between a TLC and a TV
10T6090		Timer, 8 positions

### TV2500


#### Accessories

P/N	Picture	Description																		
Thermometers		Thermometer																		
		<table border="1"> <thead> <tr> <th>ASTM no.</th> <th>Part no.</th> <th>Range°C</th> </tr> </thead> <tbody> <tr> <td>Similar to 44C</td> <td>25T0924B</td> <td>+18.5 ... +21.5</td> </tr> <tr> <td>Similar to 46C</td> <td>25T0939B</td> <td>+48.6 ... +51.4</td> </tr> <tr> <td>Similar to 47C</td> <td>25T0940B</td> <td>+ 58.6 ... +61.5</td> </tr> <tr> <td>S120C</td> <td>25T0990B</td> <td>+38.6 ... +41.4</td> </tr> <tr> <td>Similar to 121C</td> <td>25T0991B</td> <td>+98.6 ... +101.4</td> </tr> </tbody> </table>	ASTM no.	Part no.	Range°C	Similar to 44C	25T0924B	+18.5 ... +21.5	Similar to 46C	25T0939B	+48.6 ... +51.4	Similar to 47C	25T0940B	+ 58.6 ... +61.5	S120C	25T0990B	+38.6 ... +41.4	Similar to 121C	25T0991B	+98.6 ... +101.4
		ASTM no.	Part no.	Range°C																
		Similar to 44C	25T0924B	+18.5 ... +21.5																
		Similar to 46C	25T0939B	+48.6 ... +51.4																
		Similar to 47C	25T0940B	+ 58.6 ... +61.5																
S120C	25T0990B	+38.6 ... +41.4																		
Similar to 121C	25T0991B	+98.6 ... +101.4																		
Other ranges available on request																				
00T0239		Thermometer holder																		
E20 thermometer		Please see specification sheet "E20 thermometers"																		
14T0303		Adapter to insert an E20 thermometer in the opening of the cover																		
Viscosity accessories		Please see specification sheet "Viscosity accessories", e.g. viscometers, viscometer holders, bath fluids, general purpose reference standards, etc																		

TV2500

### TV2500

#### D1298 Set-up for Density Measurement by hydrometer

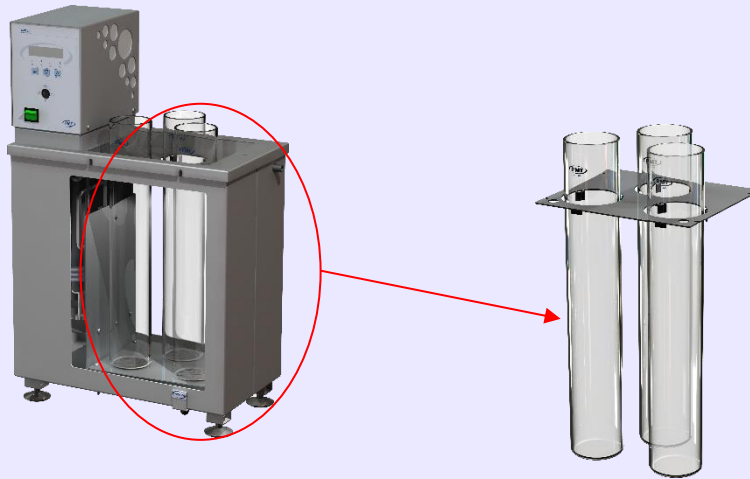

P/N	Picture	Description
03T2119		Cover with 3 openings: - 3 x $\varnothing 60.6$ mm opening - 2 x $\varnothing 12.5$ mm opening for thermometer
09T0400		Density cylinder
00T0239		Thermometer holder
00T0565		Cooling circulator TLC15-5 230V/50Hz
00T0567		Cooling circulator TLC15-5 230V/60Hz
00T0570		Cooling circulator TLC15-5 115V/60Hz
Hydrometers		Please see specification sheet "ASTM D1298"